


PHI / PII Process Flow - Acquire





Department needs to Acquire Medical Equipment

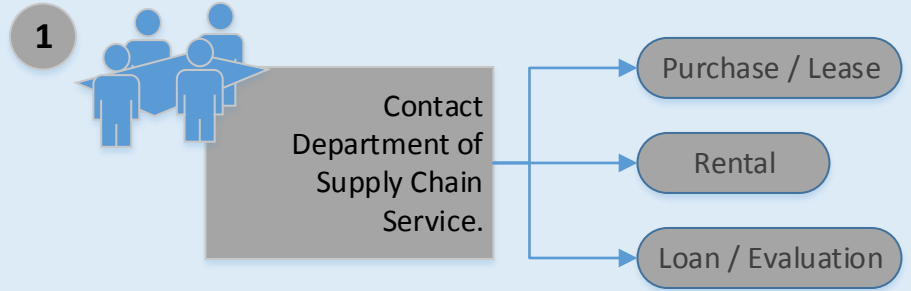

Supply Chain will develop a contract with the OEM.

2 OEM will complete a Medical Equipment PHI/PII Risk Assessment Form

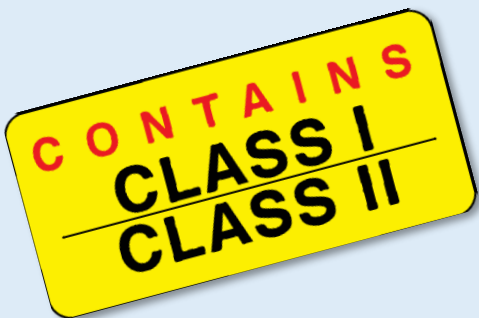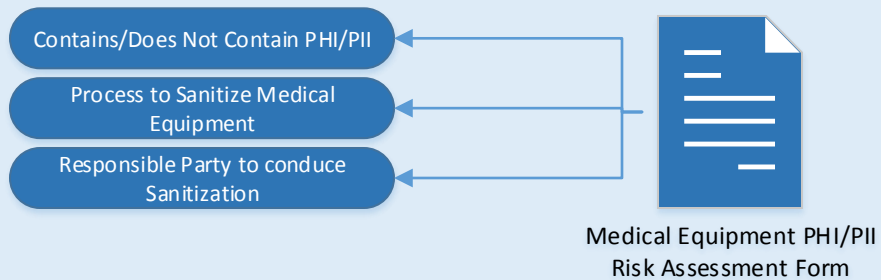

3 Department will Contact Clinical Engineering Department for Incoming Medical Inspection. If medical equipment hold PHI/PII – Will Attach Sticker

Clinical Engineering uploads documents & updates the master Medical Equipment Inventory